

Optimal PEEP in Mechanically Ventilated Patients: A Clinical Study

Sundaresan¹, J.G.Chase¹, C.E.Hann¹ and G.M.Shaw^{2,3}

1. Centre for Bioengineering, Department of Mechanical Engineering, University of Canterbury
2. Department of Intensive Care Medicine, Christchurch Hospital, New Zealand
3. Christchurch School of Medicine and Health Sciences, University of Otago, New Zealand



INTRODUCTION

OVERVIEW:


Acute Respiratory Distress Syndrome (ARDS) has mortality rates ranging from 30% to 70% [1]. Patients who are diagnosed with ARDS are often then required to undergo mechanical ventilation in the ICU; a process that can be clinically burdensome and difficult to optimise. This research examines the clinical viability of patient-specific models [2] in pilot clinical trials to assist therapy, optimise patient-specific PEEP, assess the disease state and response over time.

GOALS:

Ten patients with acute lung injury or ARDS underwent incremental PEEP recruitment manoeuvres. PV data was measured at increments of 5 cmH₂O and fitted to the recruitment model. Inspiratory and expiratory breath holds were performed to measure airway resistance and auto-PEEP. Optimal PEEP using various metrics were determined for all patients. Two patients underwent multiple recruitment manoeuvres over time and model metrics reflected and tracked the state or their ARDS.

RECRUITMENT MODEL BASICS

Alveoli recruitment and de-recruitment controlled by the normally distributed Threshold Opening Pressure (TOP) and Threshold Closing Pressure (TCP), which are assumed to be normally distributed.

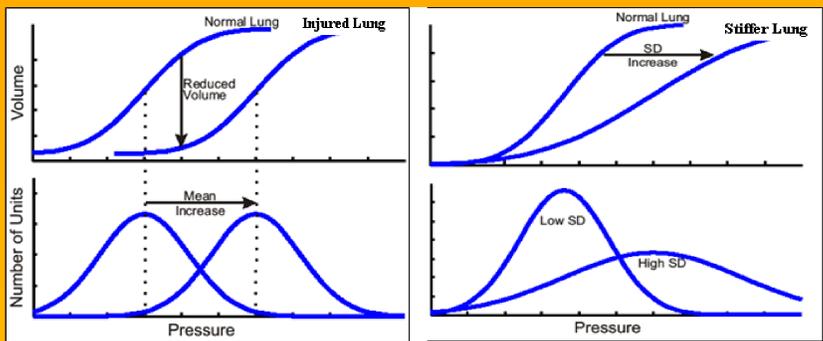



Model parameters indicate patient recruitability and lung compliance

DISEASE STATE METRICS

Metrics measured over time to assess disease state

(1) Mean Time Metric

(2) Compliance Time Metric

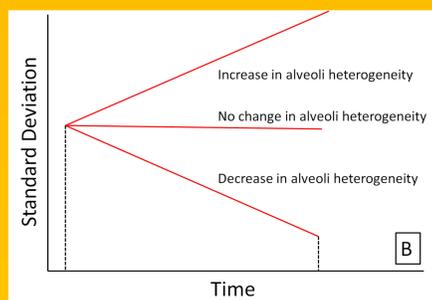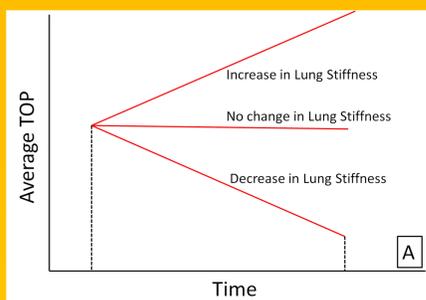

(3) TOP Gradient Metric

(4) TCP Gradient Metric




PEEP SELECTON METRICS

Metrics to optimise PEEP

(1) TOP





(2) TCP

(3) Net Recruitment

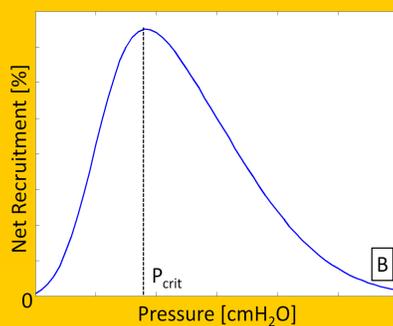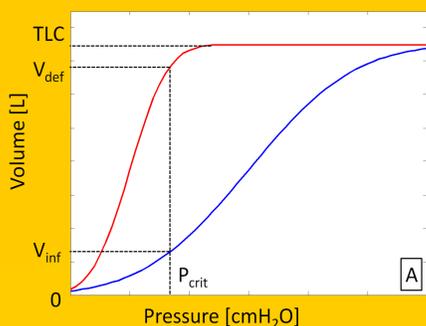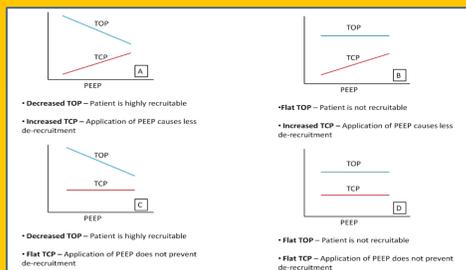

MODEL FITTING

Model was validated using PV curves from ten patients

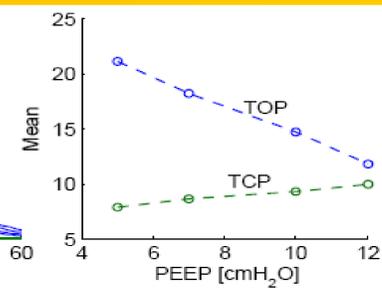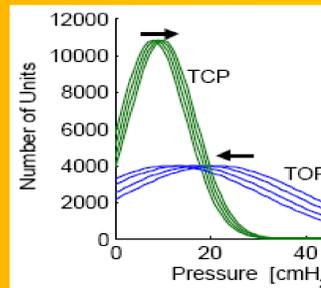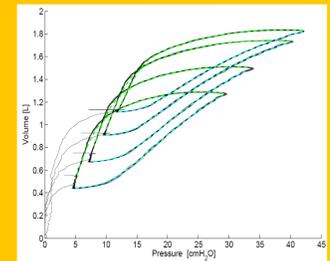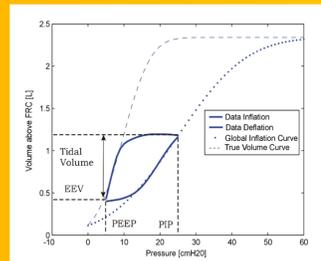

TOP / TCP average patient response

CLINICAL VIABILITY & RESULTS

- Three different metrics to help determine optimal PEEP!
 - TOP** – PEEP chosen such that, any additional pressure does not recruit additional units
 - TCP** – PEEP chosen such that at least 50% of alveoli remain recruited during expiration. Theoretically could increase PEEP, but this risks overinflating healthy units
 - Net Recruitment** – Combines the effect of TOP and TCP. PEEP chosen when net recruitment is maximised. Represents the point where additional PEEP does not recruit as many new alveoli and does not keep as many alveoli recruited

Clinically Selected PEEP [cmH ₂ O]	Model-Based PEEP Selection [cmH ₂ O]			Net Recruitment
	TOP	TCP	Net Recruitment	
Patient 1	10	27	20	20
Patient 2	12	15	15	15
Patient 3	10	10	15	20
Patient 4	10	20	20	30
Patient 5	12	20	25	25
Patient 6	11	15	20	20
Patient 7	7.5	5	10	10
Patient 8	12	15	20	30

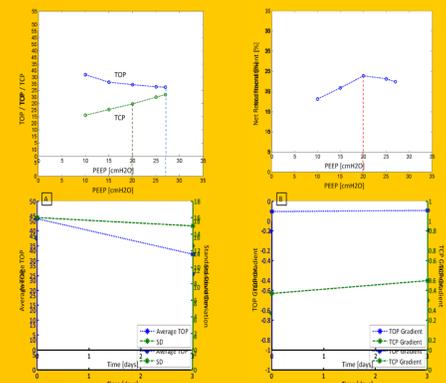


Table highlights the optimal PEEP according to model metrics. Clinically selected PEEP is significantly lower than model outputs as a compromise between efficacy and safety

Top Left - shows the TOP and TCP mean shift for Patient 1. Top Right - shows the net recruitment highlighting optimal PEEP. Bottom - Disease state metrics Patient 5

CONCLUSIONS

- 3 model-based metrics to optimise PEEP + 4 Metrics to assess disease state over time are presented and assessed
- Mechanical failure / significant compliance changes are captured by the model, however it is limited in assessing COPD patients
- Can be run with software only and using data directly from ventilators – simply, efficient, no extra invasive sensors
- Shows the potential of patient-specific modeling to provide optimised, patient-specific care (e.g. PEEP selection) within an overall protocol based on current, accepted clinical understanding and goals.
- Clearly illustrates how model parameters can create a clear physiological picture of patient-status by capturing physiologically and clinically relevant behaviours. Specifically, underlying physiological condition is represented by model parameters and their change over time (e.g. compliance)

REFERENCES

- [1] Chiumello, D. et al. (2008). "Lung Stress and Strain during Mechanical Ventilation for Acute Respiratory Distress Syndrome." *Am. J. Respir. Crit. Care Med.* 178(4): 346-355.
- [2] Sundaresan, A., Yuta, T., Hann, C. E., Geoffrey Chase, J. & Shaw, G. M. (2009). A minimal model of lung mechanics and model-based markers for optimizing ventilator treatment in ARDS patients. *Computer Methods and Programs in Biomedicine*, 95 (2): 166-180.